

Vangard® Filters



Table of Contents - Vanguard® Filters



Materials of Construction	3
Dimensions	4
Operating Characteristics	5
Cartridge Installation Instructions	6
Autoclave Instructions	7
Inline Steam Sterilization Procedure	8
Storage and Shelf Life	9
Vanguard® Media Grade Descriptions	10
Cartridge Ordering Matrix Description	11
Small Flow Elements (SFE Filters) Ordering Matrix Description	12
Capsule (CS/CL) Ordering Matrix Description	13
Capsule (CF) Ordering Matrix Description	14
Capsule (CM/CK) Ordering Matrix Description	15
UltraCap® (T-Style & Inline) Ordering Matrix Description	16
UltraCap® H.D. (T-Style & Inline) Ordering Matrix Description	17

Vangard® Filters

Vangard® is a nominal-rated PP microfiber filter that provides economical high efficiency filtration of fluids in a wide range of industrial processes. This general purpose filter delivers high flow rates with substantial dirt holding capacity for long service life. Its all-polypropylene construction provides minimal extractables and wide chemical compatibility. The Vangard® filter is a cost-effective choice for clarification, prefiltration and final filtration applications where high quality output and consistency are important.

Materials of Construction

The Vangard® filter is manufactured using high quality components made from non-toxic and biologically inert raw materials. All components of the Vangard® filter are FDA listed for food contact use in the Code of Federal Regulations (CFR), Title 21 as below:


Components

Media:	Polypropylene (PP)	CFR Title 21, 177.1520
Upstream/Downstream support:	Polypropylene	CFR Title 21, 177.1520
Core/Outer guard:	Polypropylene	CFR Title 21, 177.1520
End caps/Adaptors:	Polypropylene	CFR Title 21, 177.1520
Capsule housing:	Polypropylene	CFR Title 21, 177.1520
O-rings:	Buna, EPR or Silicone	CFR Title 21, 177.2600
	Teflon® over Silicone or	CFR Title 21, 177.1550
	Teflon® over Viton®	
Sealing method:	Thermal bonding	

The Vangard® filter complies with European Commission Regulation No. 10/2011. The filter meets requirements as specified in the current USP Class VI plastics, pyrogen and cytotoxicity tests. No binders, adhesives or surfactants are used in the construction of Vangard® filters. The filters are non-fiber-releasing as defined in 21 CFR 210.3(b)(6) and 211.72.

Configurations

Vangard® can be ordered in a variety of configurations from SFE filter cartridges through UltraCap® high capacity capsule filters.

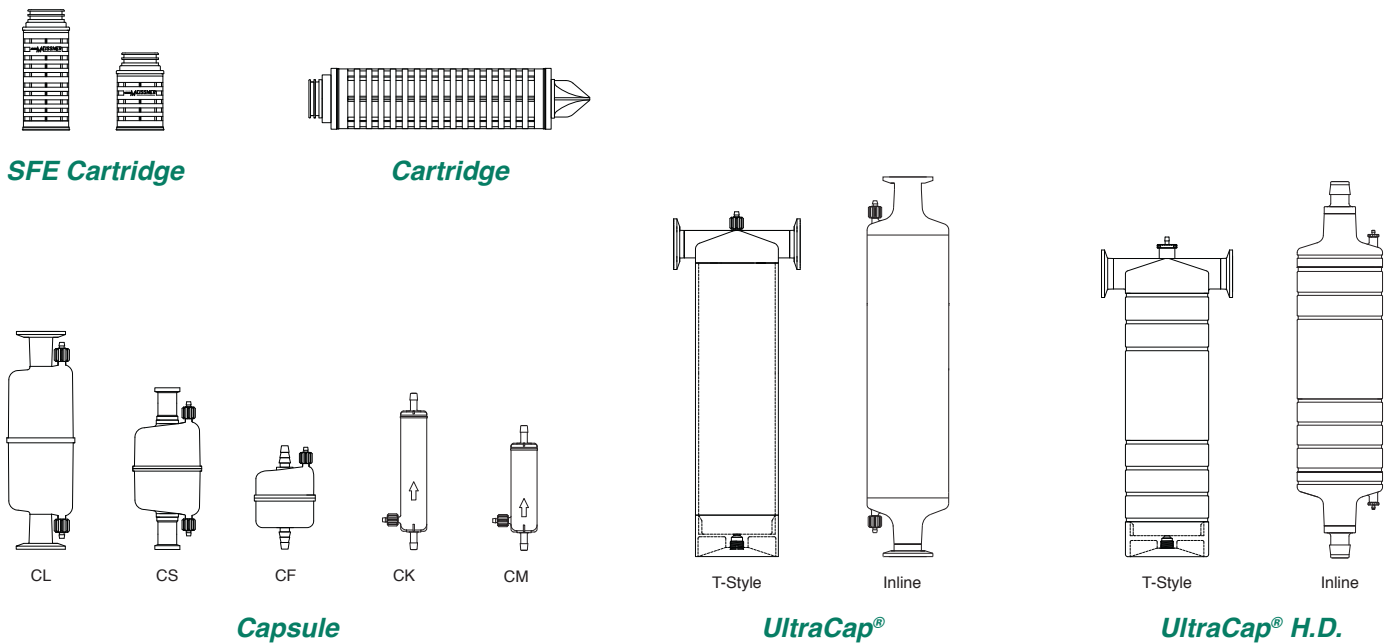


Dimensions

<i>Cartridge</i>	<i>Diameter</i>	<i>Length (nominal)</i>	<i>EFA**</i>
	2.75" (7 cm)	10" (25 cm) 20" (50 cm) 30" (75 cm) 40" (100 cm)	5.2 ft ² (0.48 m ²) 10.4 ft ² (0.97 m ²) 15.6 ft ² (1.45 m ²) 20.8 ft ² (1.93 m ²)

<i>SFE Cartridge</i>	<i>Diameter</i>	<i>Length (nominal)</i>	<i>EFA</i>
	2.25" (5.7 cm)	2.5" (6.4 cm) 5" (12.7 cm)	1.0 ft ² (0.09 m ²) 2.0 ft ² (0.19 m ²)

<i>Capsule</i>	<i>Diameter</i>	<i>Length (nominal)</i>	<i>EFA</i>
CL/CL2	2.75" (7.0 cm)	6.9" (17.5 cm)	2.0 ft ² (0.19 m ²)
CS/CS2	2.75" (7.0 cm)	4.5" (11.4 cm)	1.0 ft ² (0.09 m ²)
CF/CF2-A	2.25" (5.7 cm)	3.3" (8.3 cm)	0.33 ft ² (305 cm ²)
CF/CF2-B	2.25" (5.7 cm)	3.3" (8.3 cm)	0.50 ft ² (465 cm ²)
CK2	1.15" (2.9 cm)	6.25" (15.9 cm)	0.36 ft ² (335 cm ²)
CM2	1.15" (.9 cm)	5.50" (14.0 cm)	0.29 ft ² (270 cm ²)

<i>UltraCap®</i>	<i>Diameter *</i>	<i>Length (nominal)</i>	<i>Capsule Dimension (overall)</i>	<i>EFA</i>
T-style	3.25" (8 cm)	10" (25 cm) 20" (50 cm) 30" (75 cm)	12.3" (31,2 cm) 22.3" (56,6 cm) 32.3" (82 cm)	5.2 ft ² (0.48 m ²) 10.4 ft ² (0.7 m ²) 15.6 ft ² (1.45 m ²)
Inline	3.25" (8 cm)	10" (25 cm) 20" (50 cm) 30" (75 cm)	14.8" (37. cm) 24.9" (63.2 cm) 34.9" (88.6 cm)	5.2 ft ² (0.48 m ²) 10.4 ft ² (0.97 m ²) 15.6 ft ² (1.45 m ²)



<i>UltraCap® H.D.</i>	<i>Diameter *</i>	<i>Length (nominal)</i>	<i>Capsule Dimension (overall)</i>	<i>EFA</i>
T-style	3.5" (9 cm)	10" (25 cm) 20" (50 cm) 30" (75 cm) 40" (100 cm) 50" (125 cm)	11.7" (29.7 cm) 21.1" (53.6 cm) 30.6" (77.7 cm) 40.0" (101.6 cm) 49.5" (125.7 cm)	5.2 ft ² (0.48 m ²) 10.4 ft ² (0.97 m ²) 15.6 ft ² (1.45 m ²) 20.8 ft ² (1.93 m ²) 26.0 ft ² (2.2 m ²)
Inline	3.5" (9 cm)	10" (25 cm) 20" (50 cm) 30" (75 cm) 40" (100 cm) 50" (125 cm)	17.3" (43.9 cm) 26.8" (68.1 cm) 36.2" (91.9 cm) 45.7" (116.1 cm) 55.2" (140.2 cm)	5.2 ft ² (0.48 m ²) 10.4 ft ² (0.97 m ²) 15.6 ft ² (1.45 m ²) 20.8 ft ² (1.93 m ²) 26.0 ft ² (2.42 m ²)



*Inlet/outlet fittings extend beyond stated diameter

**EFA = Effective Filtration Area

Operating Characteristics

Cartridges and SFE (Small Flow Elements)

Maximum Operating Temperatures and Pressures
80 psid @ 32 °F to 100 °F
(Δp 5.5 bar @ 0 °C to 38 °C)

60 psid @ 150 °F
(Δp 4.1 bar @ 66 °C)

30 psid @ 180 °F
(Δp 2.1 bar @ 82 °C)

Capsules - CS/CL & CF Models

Maximum Operating Pressure, Liquids
75 psig @ 32 °F to 100 °F
(5.2 bar @ 0 °C to 38 °C)

Maximum Operating Temperature Rating
160 °F @ 35 psig
(71 °C @ 2.4 bar)

Maximum Operating Pressure, Gas
50 psig @ 32 °F to 100 °F
(3.4 bar @ 0 °C to 38 °C)

Capsules - CM/CK Models

Maximum Operation Pressure & Temperature, Liquids
100 psig @ 32 °F to 122 °F
(6.9 bar @ 0 °C to 50 °C)

Maximum Operating Pressure & Temperature, Gas
100 psig @ 32 °F to 122 °F
(6.9 bar @ 0 °C to 50 °C)

UltraCap® Model

Maximum Operating Pressure & Temperature, Liquids
75 psig @ 32 °F to 100 °F
(5.2 bar @ 0 °C to 38 °C)

45 psig @ 140 °F
(3.1 bar @ 60 °C)

Maximum Operating Pressure & Temperature, Gas
50 psig @ 32 °F to 100 °F
(3.4 bar @ 0 °C to 38 °C)

30 psig @ 140 °F
(2.1 bar @ 60 °C)

UltraCap® H.D. Model

Maximum Operating Pressure & Temperature, Liquids
90 psig @ 32 °F to 100 °F
(6.2 bar @ 0 °C to 38 °C)

55 psig @ 140 °F
(3.8 bar @ 60 °C)

Maximum Operating Pressure & Temperature, Gas
60 psig @ 32 °F to 100 °F
(4.1 bar @ 0 °C to 38 °C)

35 psig @ 140 °F
(2.4 bar @ 60 °C)

Cartridge Installation Instructions

Meissner filters are available in a number of different adapter and O-ring configurations designed to fit modern filter housings. The filter should fit snugly in the housing. Improper installation can impair filtration efficiency.

1. Verify that the correct filter part number for the application has been chosen.
2. Keep the filter in its plastic bag to avoid contaminating the cartridge as long a possible. Cut open the bag at the O-ring end. While holding the bagged cartridge, lubricate the O-rings by dipping the O-rings into clean water or other suitable liquid compatible with the process fluid.
3. Line up the open end of the cartridge with the housing seat and install using a slight twisting motion while holding the bagged cartridge near the O-ring adapter. Verify that the O-rings are fully seated and not twisted. If the cartridge has locking tabs, rotate the tabs into place with a clockwise motion until engaged. Caution: always rotate cartridges while firmly grasping the O-ring end of the cartridge to prevent excessive torque damage to the filter.
4. Repeat with additional cartridges. Remove protective bags from the cartridges. If present, install cartridge retainer system (plate or spring). Reassemble housing.

Autoclave Instructions

Meissner filters may be autoclaved repeatedly without loss of integrity.

Capsule, UltraCap® and UltraCap® H.D. Filters

The following outlines the steps recommended in the autoclave sterilization of Meissner filter capsules.

1. Loosely cover the capsule inlet and outlet with autoclave wrap. All capsule vents are on the upstream side of the filter and should be loosened or removed to facilitate steam penetration. Hose barb vent valves must be opened at least two full turns to prevent valve leakage post autoclaving.
2. The weight of clamps or fittings attached to the capsule must be supported to avoid damaging the adapters. Sanitary flanges may have clamps and gaskets loosely attached to the filter. If fittings must be attached to flanges, tri-clamps are preferable to bi-clamps and should be tightened after the assembly has cooled.
3. Autoclave the capsule at a minimum of 121 °C for 60 minutes or 125 °C for at least 45 minutes with the capsule in a horizontal position using a slow exhaust or liquid cycle. T-style UltraCap® capsules may be autoclaved horizontally or with the outlet oriented downward to facilitate the removal of condensate from the downstream side of the filter. As autoclave systems vary, sterilization cycles should be validated under actual system or autoclave loading conditions. Downstream attachments can significantly increase the time required to sterilize the filter core.
4. Allow the capsule to cool. Gently close vents finger tight. Excessive tightening of vent valves will damage the sealing surfaces. Integrity test if desired. Install filter into system aseptically.

Cartridge and SFE (Small Flow Elements)

The following outlines the steps required to autoclave a Meissner filter cartridge and housing assembly. A stainless steel reinforcement ring is required for filter configurations with 222 or 226 O-rings.

1. Install the filter into the housing. Loosely cover the inlet and outlet with autoclave wrap. Vent and drain valves should be fully open.
2. Autoclave the cartridge and housing assembly at a minimum of 121 °C for 30 minutes with the filter outlets in an outlet down or horizontal position using a slow exhaust or liquid cycle. As autoclave systems vary, sterilization cycles should be validated under actual system or autoclave loading conditions. Assemblies attached to the outlet can increase the required sterilization times.
3. Allow the housing assembly to cool.
4. Install the sterile filter assembly into the system using aseptic techniques.

Different autoclave temperature and time combinations may be used to sterilize the filters but the combination should be validated to ensure that sterilization occurs under those conditions. Temperatures above 135 °C are not recommended.

Inline Steam Sterilization Procedure

Steaming in place (SIP) is frequently used in critical applications where a sterile effluent is desired. To prevent damage to the filter cartridge's O-ring adapter, cartridges with 222 or 226 O-rings must be reinforced with a stainless steel ring. Meissner filter cartridges with reinforced O-ring adapters are capable of repeated sterilization cycles without loss of integrity. The steps required to steam sterilize a Meissner filter cartridge and system using saturated steam are outlined in the procedure, below.

The steam should be free of rust and other particulates. The housing should be clean before the cartridge is installed. If you are steam sterilizing a wetted cartridge, upstream and downstream gauges must be provided to verify that the differential pressure across the filter does not exceed 5 psi (0,3 bar). To assure sterilization, steam pressure in the assembly must not be allowed to fall below 15 psi (1 bar or 121 °C). Condensate should be drained from the system during sterilization. A typical piping schematic is outlined in Figure 1.

Caution: Capsules, UltraCap® and UltraCap® H.D. are not designed for inline steam sterilization!

Procedure (Figure 1)

1. Close all valves.
2. Open valve V_4 .
3. If cartridge is wet, or if there is a large volume tank downstream of the filter, open V_5 .
 - a. Slowly open V_2 . This will connect both sides of the filter to steam pressure.
 - b. Crack open V_7 to vent trapped air.
 - c. Crack open V_6 allowing steam to flow through the system.
 - d. Slowly close V_5 but do not allow the differential pressure across the cartridge to exceed 5 psi (0,3 bar).
 - e. Leave drain V_8 cracked during sterilization to drain condensate.
4. If sterilizing a dry cartridge, slowly open V_2 .
 - a. Crack open V_7 to vent trapped air.
 - b. Crack open V_6 to allow steam to flow through the system. Do not allow the differential pressure across the cartridge to exceed 5 psi (0,3 bar).
 - c. Leave drain V_8 cracked during sterilization to drain condensate.
5. Steam sterilize for 30 to 60 minutes at 15 to 20 psig (1,0 to 1,4 bar), or as long as experience dictates.
6. When sterilization is complete, close V_2 .
7. Open V_3 and introduce sterile air or nitrogen regulated to the same pressure as the steam.
8. Close V_8 once steam and condensate flow stops.
9. Allow the system to cool to room temperature. Do not allow the differential pressure across the cartridge to exceed 5 psi (0,3 bar). Then close V_3 , V_7 and V_6 . Keep the system under pressure until ready for use.
10. Crack vent V_7 and allow the system pressure to equalize. The filtration process may now be started.

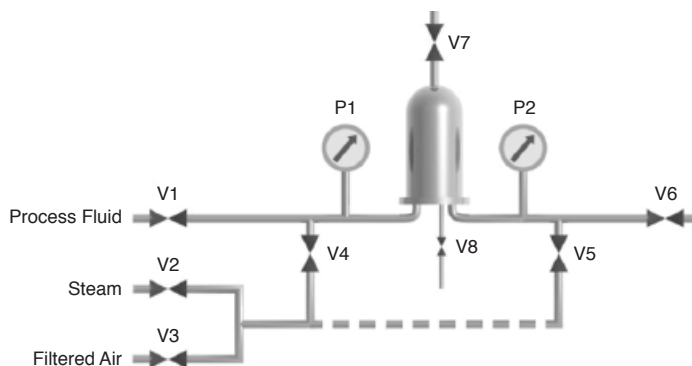


Figure 1

Storage and Shelf Life

Meissner manufactures a complete line of filter products and One-Touch® single use assemblies. Products are suitably bagged and boxed for shipping and may be stored in the original packaging in a clean dry area between 0 °C and 40 °C (32 °F to 100 °F). The following gives the minimum shelf life expectancies for Vanguard® products.

Filters

The Vanguard® filter has an expected shelf life greater than 5 years in the cartridge, small flow, large and small capsule lines, and disc configurations. Filters may be used beyond their minimum expected shelf life if they were stored in their original packaging and are integrity tested prior to use and found to be within specification. Filter product age can be determined from the date on the original Certificate of Quality or Conformance.

One-Touch® Products

The One-Touch® product line of single-use systems, including but not limited to biocontainers, tubing, and/or filter assemblies, has labeling which identifies the product specific expiration date. The standard shelf life of nonsterile One-Touch® products is 2 years from the date of manufacture. These standard time periods may be amended to reflect the various components included in a specific configuration, a change that will be indicated on the product label.

Vangard® Media Grade Description

MN = This pleated, depth type filter is constructed entirely of chemically resistant polypropylene. A Certificate of Conformance is available on a lot basis.

Cartridge Ordering Matrix Description

MN	0.1	—	2	C6	R	S
MN		—				
Filter Grade	Nominal Rating (µm)	—	Cartridge Length	End Cap Configuration	Reinforcement Ring Option	Seal Material (O-ring or Gasket)
MN	0.1 0.2, 0.4, 1, 3, 5, 10, 30, 60, 99		1 = 10" 2 = 20" 3 = 30" 4 = 40"	GS = DOE; flat gaskets (9.75", 19.5", 29.25", 39" length filters) GL = DOE; flat gaskets (20", 30", 40" length filters) C1 = SOE; 222 nO-Ring®, button cap end C2 = SOE; 222 O-rings, button cap end F1 = SOE; 222 nO-Ring®, fin end F2 = SOE, 222 O-rings, fin end C5 = SOE; 226 nO-Ring®, button cap end C6 = SOE; 226 O-rings, button cap end F5 = SOE; 226 nO-Ring®, fin end Vanguard® Filters F6 = SOE; 226 O-rings, fin end DN = DOE; internal 120 O-rings RN = SOE; internal 120 O-ring, recessed cap end DA = DOE; internal 213 O-rings RA = SOE; internal 213 O-ring, recessed cap end	(Blank) = Standard - no reinforcement ring R = Reinforcement ring required for autoclave/SIP applications	<u>O-ring Seal</u> B = Buna E = EPR S = Silicone T = Teflon® over Silicone V = Viton® X = Teflon® over Viton® <u>Gasket Seal</u> B = Buna E = EPR P = Polyethylene S = Silicone T = Teflon® V = Viton®

Small Flow Elements (SFE Filters) Ordering Matrix Description

L	MN	0.1	—	5	6	R	S
L	MN		—				
Model	Filter Grade	Nominal Rating (μm)	—	Filter Length/(Area) nominal	Adapter Selection	Reinforcement Ring Option	O-ring Material
L	MN	0.1, 0.2, 0.4, 1, 3, 5, 10, 30, 60, 99		2 = 2.5"/1.0 ft² (0.09 m²) 5 = 5.0"/2.0 ft² (0.19 m²)	P = Standard internal 116 O-ring 2 = 222 O-rings (for autoclave/SIP applications, select "R" under "Reinforcement Ring Option") 6 = 226 O-ring style locking adapter (for autoclave/SIP applications, select "R" under "Reinforcement Ring Option") SK = Skirt-flange adapter (no reinforcement or O-ring options available) L = 116 O-ring with Mini Lock	(Blank) = Standard - no reinforcement ring R = Reinforcement ring - required only for the 222 and 226 adapter when autoclaving or steam sterilizing	B = Buna E = EPR S = Silicone T = Teflon® over Silicone V = Viton® X = Teflon® over Viton®

Capsule (CS/CL) Ordering Matrix Description

C	S	2	MN	0.1	—	02	2
C			MN		—		
Model	Filtration Area (nominal)	Material Code	Filter Grade	Nominal Rating (µm)		Inlet/Outlet Connections	Vent/Drain Ports
C	S = 1.0 ft² (0.09 m²) L = 2.0 ft² (0.19 m²)	(Blank) or 1 = Polypropylene capsule shell material 2 = Animal component free polypropylene capsule shell material	MN	0.1, 0.2, 0.4, 1, 3, 5, 10, 30, 60, 99		00 = 1" sanitary flange 02 = 1" sanitary flange inlet; 3/8" hose barb outlet 0C = 1" sanitary flange inlet; 1/2" hose barb outlet 22 = 3/8" hose barb 2B = 3/8" hose barb with filling bell CC = 1/2" hose barb 44 = 1/4" MNPT 55 = 3/8" FNPT 66 = 3/8" MNPT 77 = 3/4" sanitary flange 88 = 3/4" hose barb 99 = 1/2" hose barb flexible tubing	0 = No vent/drain port 1 = 1 luer port with cap, outlet side 2 = Standard - 2 luer ports with caps 4 = 2 sanitary valves with hose barb 5 = 1 sanitary valve with hose barb connection, outlet side 6 = 1 sanitary valve with hose barb connection, inlet side

Capsule (CF) Ordering Matrix Description

CF	2	MN	0.1	—	33	A	1
CF		MN		—			
Model	Material Code	Filter Grade	Nominal Rating (µm)	—	Inlet/Outlet Connections	Filtration Area (nominal)	Vent/Drain Ports
CF	(Blank) or 1 = Polypropylene capsule shell material 2 = Animal component free polypropylene capsule shell material	MN	0.1, 0.2, 0.4, 1, 3, 5, 10, 30, 60, 99		33 = Hose barb (1/4" - 3/8") 3B = Hose barb (1/4" - 3/8") with filling bell 41 = 1/4" MNPT inlet; 1/4" hose barb outlet 44 = 1/4" MNPT 77 = 3/4" sanitary flange	A = 0.33 ft² (305 cm²) B = 0.50 ft² (465 cm²)	0 = No vent/drain port 1 = Standard - 1 luer port with cap, outlet side 2 = 2 luer ports with caps 4 = 2 sanitary valves with hose barbs 5 = 1 sanitary valve with hose barb connection, inlet side

Capsule (CM/CK) Ordering Matrix Description

C	K	2	MN	0.1	—	77	4
C		2	MN		—		
Model	Filtration Area (nominal)	Material Code	Filter Grade	Nominal Rating (μm)	—	Inlet/Outlet Connections	Vent/Drain Ports
C	M = 0.29 ft² (270 cm²) K = 0.36 ft² (335 cm²)	2 = Animal component free polypropylene capsule shell material	MN	0.1, 0.2, 0.4, 1, 3, 5,10, 30, 60, 99		11 = 1/4" hose barb 1B = 1/4" hose barb w/ filling bell 22 = 3/8" hose barb 2B = 3/8" hose barb w/ filling bell 41 = 1/4" MNPT; 1/4" hose barb out 44 = 1/4" MNPT 71 = 3/4" TC in; 1/4" hose barb out 72 = 3/4" TC in; 3/8" hose barb out 77 = 3/4" sanitary (TC) flange	0 = No vent/drain port 1 = 1 luer port with cap, inlet side 2 = Standard - 2 luer ports with caps 4 = 2 sanitary valves with hose barb 5 = 1 sanitary valve with hose barb connection, inlet side 6 = 1 sanitary valve with hose barb, outlet side

UltraCap® (T-Style & Inline) Ordering Matrix Description

CU	MN	0.1	—	2	T	00	2
CU	MN		—				
Model	Filter Grade	Nominal Rating (µm)	—	Cartridge Length	Body Style	Inlet/Outlet Connections	Vent/Drain Ports T-Style
CU	MN	0.1, 0.2, 0.4, 1, 3, 5, 10, 30, 60, 99		1 = 10" 2 = 20" 3 = 30"	T = T-style N = Inline	00 = 1" sanitary flange 77 = 3/4" sanitary flange 02 = 1" sanitary flange inlet; 3/8" hose barb outlet 0C = 1" sanitary flange inlet; 1/2" hose barb outlet 09 = 1" sanitary flange inlet; 9/16" hose barb outlet 08 = 1" sanitary flange inlet; 3/4" hose barb outlet 22 = 3/8" hose barb CC = 1/2" hose barb 99 = 9/16" hose barb 88 = 3/4" hose barb AA = 1/2" Flaretek® BB = 3/4" Flaretek®	0 = No vent or drain 1 = No vent; 1/4" sanitary drain plug 2 = Sanitary vent; 1/4" sanitary drain plug 3 = Sanitary vent; 3/4" sanitary flange gauge port; 1/4" sanitary drain plug 4 = Sanitary vent; no drain 5 = Sanitary vent; 3/4" sanitary flange gauge port; no drain 6 = No vent or drain; 3/4" sanitary flange gauge port
							Vent/Drain Ports Inline
							0 = No vent or drain 2 = Two sanitary vent/drain valves 4 = One sanitary vent or drain valve, outlet side

UltraCap® H.D. (T-Style & Inline) Ordering Matrix Description

CR	2	MN	0.1	—	2	T	00	2
CR	2	MN		—				
Model	Material Code	Filter Grade	Nominal Rating (µm)	—	Cartridge Length	Body Style	Inlet/Outlet Connections	Vent/Drain Ports T-Style
CR	2 = Animal component free polypropylene capsule shell material	MN	0.1, 0.2, 0.4, 1, 3, 5, 10, 30, 60, 99		1 = 10" 2 = 20" 3 = 30" 4 = 40" 5 = 50"	T = T-style N = Inline	00 = 1" sanitary flange 77 = 3/4" sanitary flange 02 = 1" sanitary flange inlet; 3/8" hose barb outlet 0C = 1" sanitary flange inlet; 1/2" hose barb outlet 09 = 1" sanitary flange inlet; 9/16" hose barb outlet 08 = 1" sanitary flange inlet; 3/4" hose barb outlet 0D = 1" sanitary flange inlet; 1" hose barb outlet 22 = 3/8" hose barb CC = 1/2" hose barb 99 = 9/16" hose barb 88 = 3/4" hose barb DD = 1" hose barb AA = 1/2" Flaretek® BB = 3/4" Flaretek®	0 = No vent or drain 1 = No vent; 1/4" sanitary drain plug 2 = Sanitary vent; 1/4" sanitary drain plug 3 = Sanitary vent; 3/4" sanitary flange gauge port; 1/4" sanitary drain plug 4 = Sanitary vent; no drain 5 = Sanitary vent; 3/4" sanitary flange gauge port; no drain 6 = No vent or drain; 3/4" sanitary flange gauge port A = No vent; sanitary drain valve B = Sanitary vent; sanitary drain valve C = Sanitary vent; sanitary drain; 3/4" sanitary flange gauge port
								Vent/Drain Ports Inline
								0 = No vent or drain 2 = Two sanitary vent/drain valves 4 = One sanitary vent or drain valve, outlet side

Viton and Teflon are registered trademarks of E. I. du Pont de Nemours and Company.
Flaretek is a registered trademark of Entegris, Inc.

Vanguard, UltraCap and UltraCap H.D. are registered trademarks of Meissner Filtration Products, Inc.
© 2025, 2013, 2007 Meissner Filtration Products, Inc.
GD009-4.0